


# Validation Data Sheet

dPCR CNV Probe Assay	HSPA9
Assay Catalog No.	DCG0000019
dPCR Instrument	QIAcuity digital PCR instrument
dPCR Master Mix	QIAcuity Probe PCR Master Mix
Experimental Sample(s)	genomic DNA, XbaI-digested

**1D Scatter Plot:** Single-well data of target assay HSPA9 (Green Channel) and reference assay TERT (Yellow Channel) in different gDNA input amounts (A7,B7,C7: 6ng/rxn, D7,E7,F7: 4ng/rxn, G6,H6: NTCs)

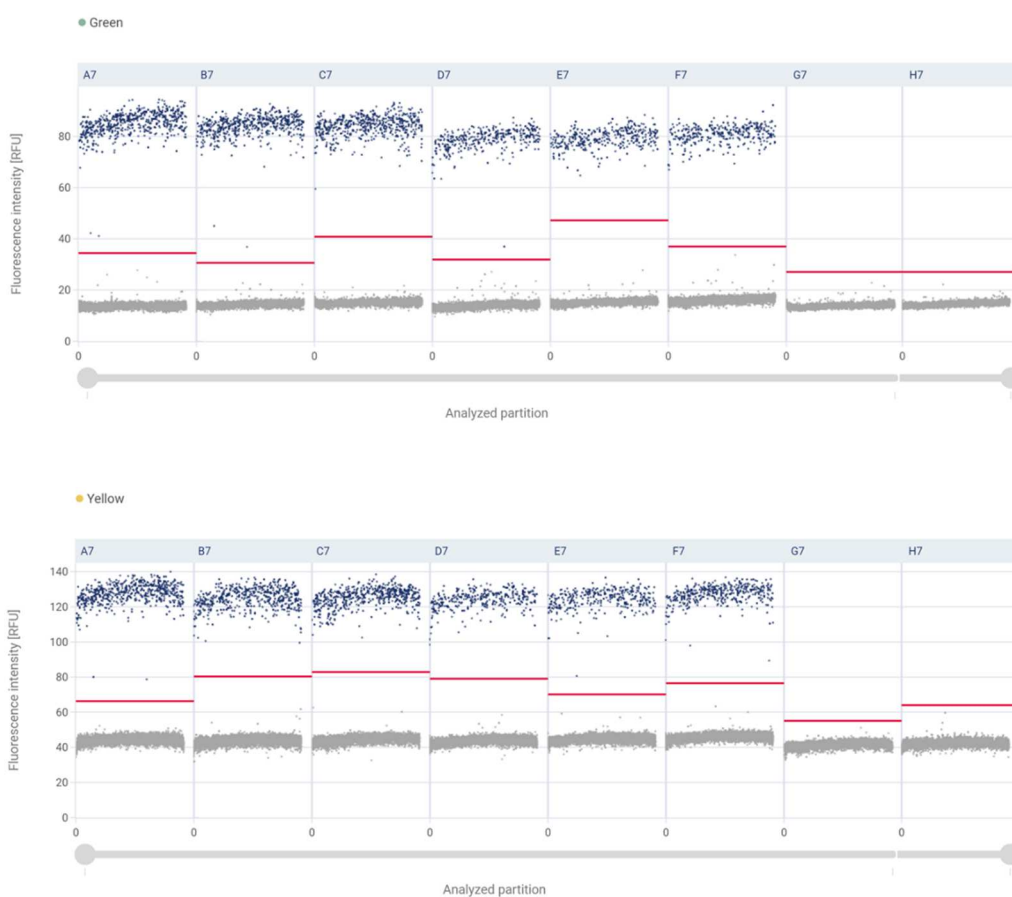

**2D Scatter Plot:** Single-well data of target assay HSPA9 (Green Channel, X-axis) and reference assay TERT (Yellow Channel, Y-axis) in 4ng gDNA input amount.

