
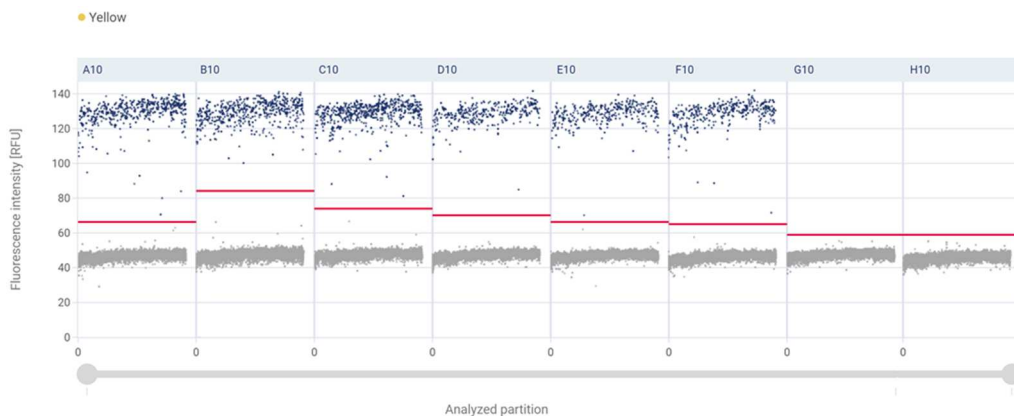


Validation Data Sheet

dPCR CNV Probe Assay	SLIT2
Assay Catalog No.	DCG0000034
dPCR Instrument	QIAcuity digital PCR instrument
dPCR Master Mix	QIAcuity Probe PCR Master Mix
Experimental Sample(s)	genomic DNA, XbaI-digested

1D Scatter Plot: Single-well data of target assay SLIT2 (Green Channel) and reference assay TERT (Yellow Channel) in different gDNA input amounts (A10,B10,C10: 6ng/rxn, D10,E10,F10: 4ng/rxn, G10,H10: NTCs)

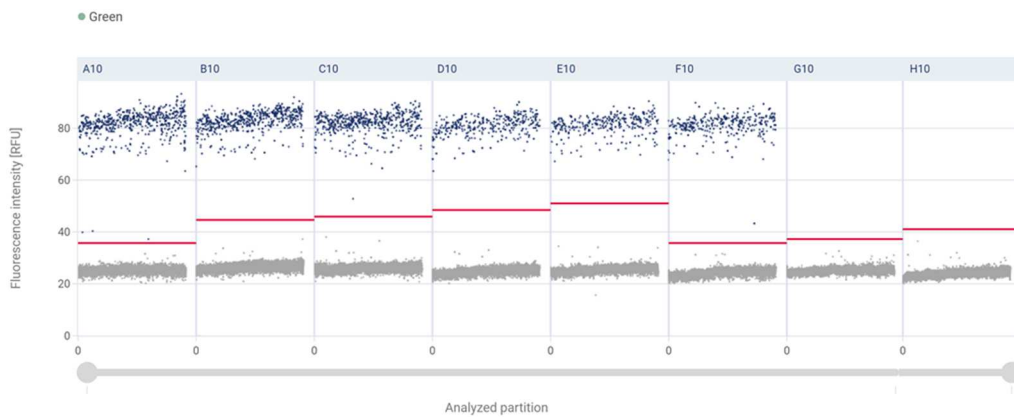

2D Scatter Plot: Single-well data of target assay SLIT2 (Green Channel, X-axis) and reference assay TERT (Yellow Channel, Y-axis) in 4ng gDNA input amount.

