
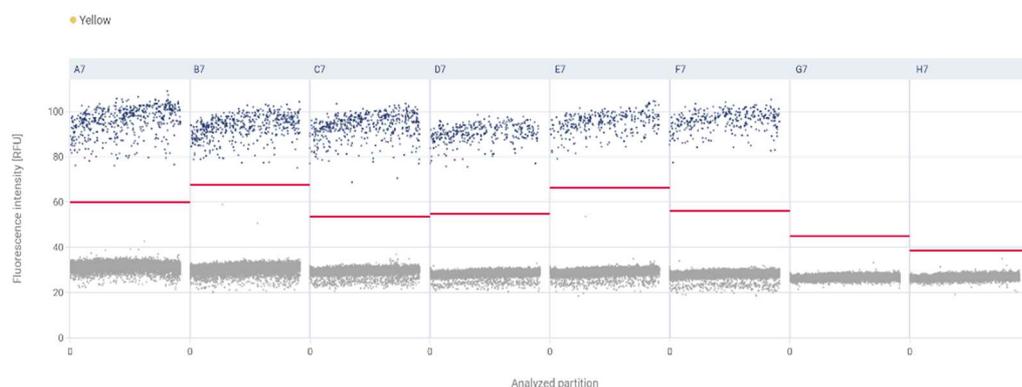


# Validation Data Sheet

<b>dPCR CNV Probe Assay</b>	<b>MAG11</b>
Assay Catalog No.	DCG0000038
dPCR Instrument	QIAcuity digital PCR instrument
dPCR Master Mix	QIAcuity Probe PCR Master Mix
Experimental Sample(s)	genomic DNA, XbaI-digested

**1D Scatter Plot:** Single-well data of target assay MAG11 (Green Channel) and reference assay AP3B1 (Yellow Channel) in different gDNA input amounts (A7,B7,C7: 6ng/rxn, D7,E7,F7: 4ng/rxn, G7,H7: NTCs)

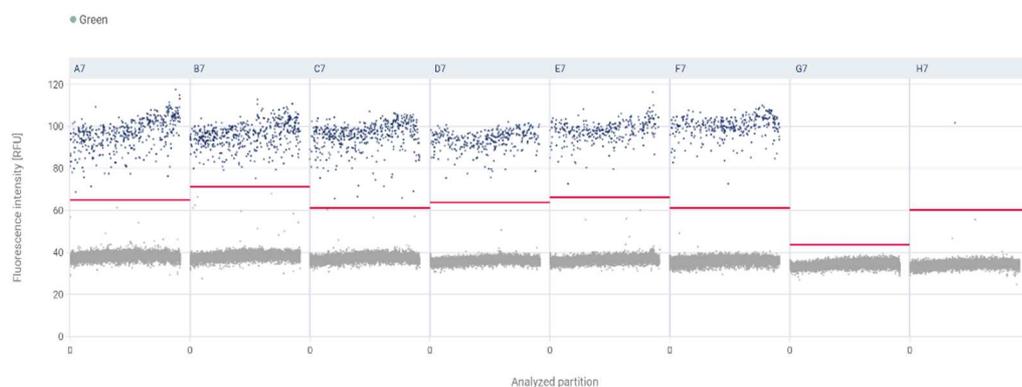

**2D Scatter Plot:** Single-well data of target assay MAGI1 (Green Channel, X-axis) and reference assay AP3B1 (Yellow Channel, Y-axis) in 4ng gDNA input amount.

