
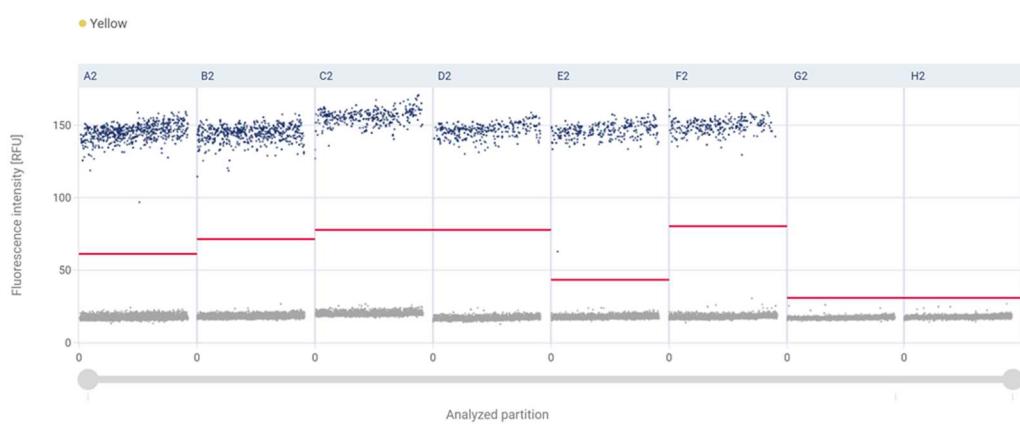


Validation Data Sheet

dPCR CNV Probe Assay	RUNX1T1
Assay Catalog No.	DCG000065
dPCR Instrument	QIAcuity digital PCR instrument
dPCR Master Mix	QIAcuity Probe PCR Master Mix
Experimental Sample(s)	genomic DNA, XbaI-digested

1D Scatter Plot: Single-well data of target assay RUNX1T1 (Green Channel) and reference assay RPP30 (Yellow Channel) in different gDNA input amounts (A2,B2,C2: 6ng/rxn, D2,E2,F2: 4ng/rxn, G2,H2: NTCs)

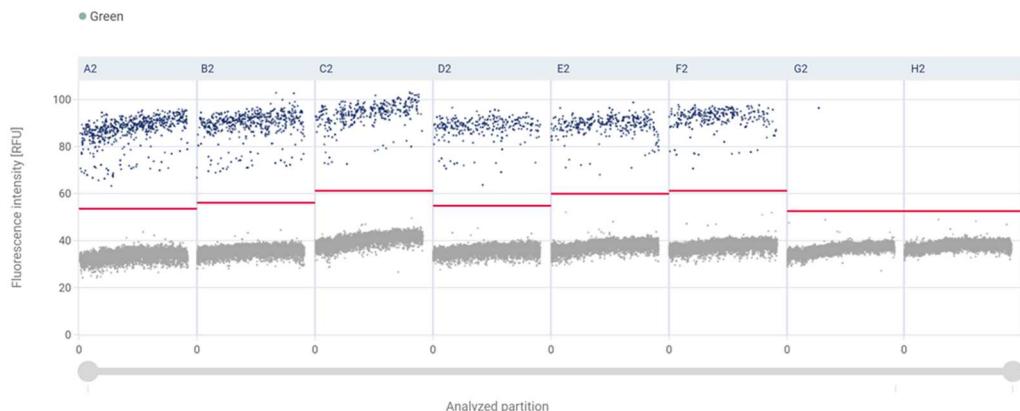

2D Scatter Plot: Single-well data of target assay RUNX1T1 (Green Channel, X-axis) and reference assay RPP30 (Yellow Channel, Y-axis) in 4ng gDNA input amount.

