
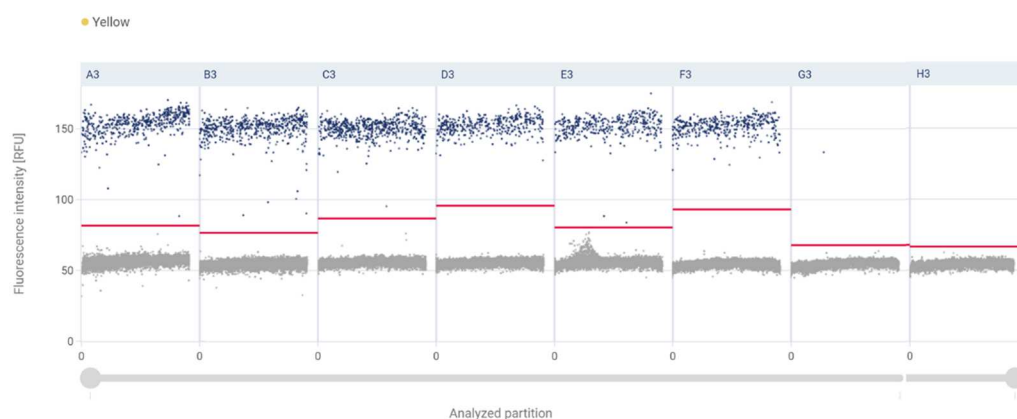


# Validation Data Sheet

<b>dPCR CNV Probe Assay</b>	<b>ETS2</b>
Assay Catalog No.	DCG0000422
dPCR Instrument	QIAcuity digital PCR instrument
dPCR Master Mix	QIAcuity Probe PCR Master Mix
Experimental Sample(s)	genomic DNA, XbaI-digested

**1D Scatter Plot:** Single-well data of target assay ETS2 (Green Channel) and reference assay TERT (Yellow Channel) in different gDNA input amounts (A10,B10,C10: 6ng/rxn, D10,E10,F10: 4ng/rxn, G10,H10: NTCs)

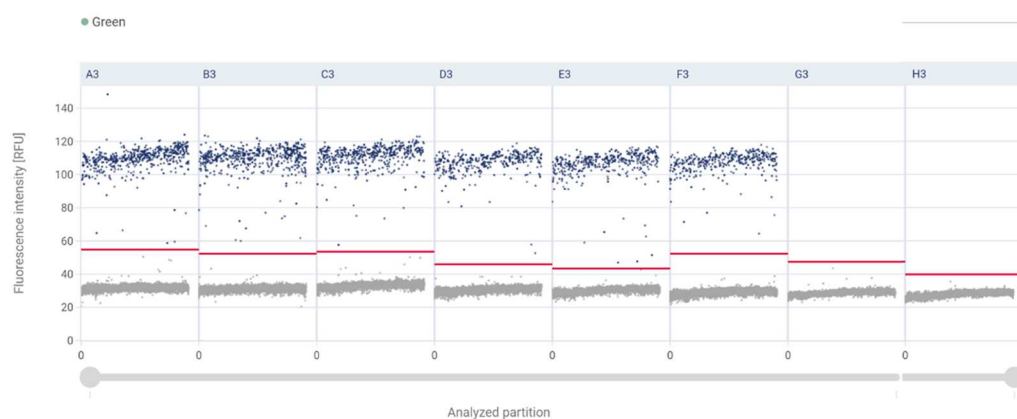

**2D Scatter Plot:** Single-well data of target assay ETS2 (Green Channel, X-axis) and reference assay TERT (Yellow Channel, Y-axis) in 4ng gDNA input amount.

