

dPCR CNV Probe Assay

Validation Data Sheet

dPCR CNV Probe Assay

MTOR

Assay Catalog No.

DCG0000594

dPCR Instrument

QIAcuity® digital PCR instrument

dPCR Master Mix

QIAcuity Probe PCR Master Mix

Experimental Sample(s)

genomic DNA, *EcoRI*-digested

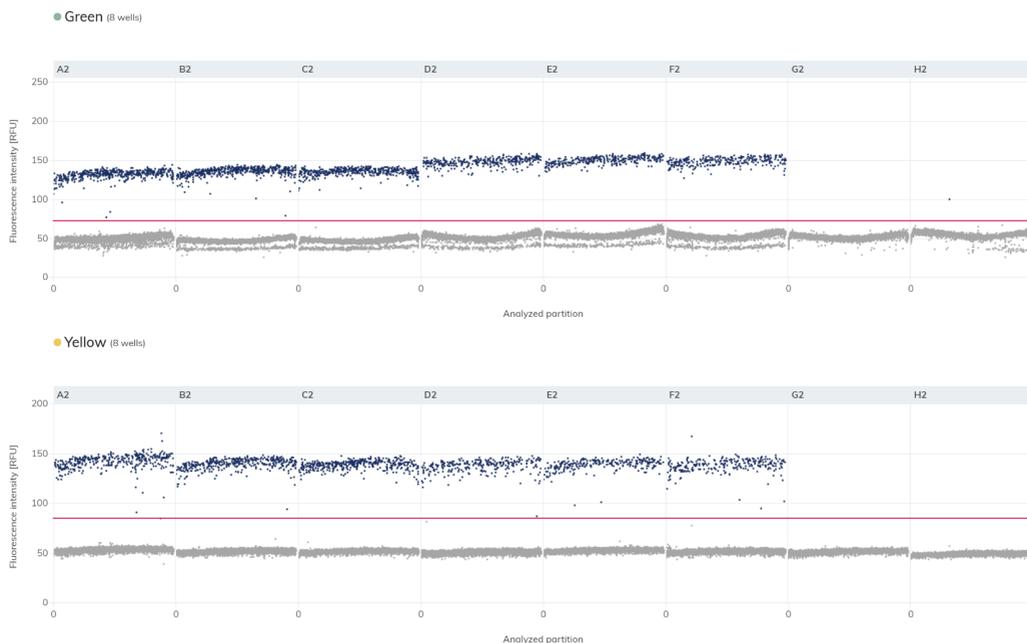


Figure 1. 1D Scatter Plot. Single-well data of target assay MTOR (Green Channel) and reference assay TERT (Yellow Channel) in different gDNA input amounts (A2, B2, C2: 6 ng/rxn; D2, E2, F2: 4 ng/rxn; G2, H2: NTCs).

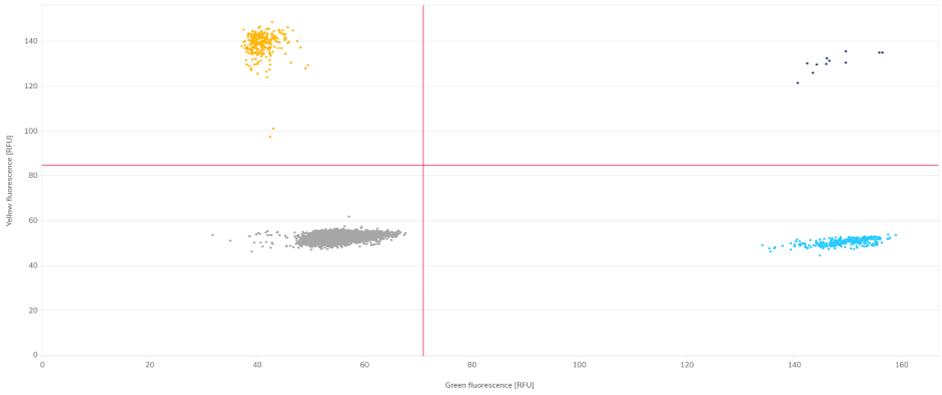


Figure 2. 2D Scatter Plot. Single-well data of target assay MTOR (Green Channel, X-axis) and reference assay TERT (Yellow Channel, Y-axis) in 4 ng gDNA input amount.